


# Erratum to: Efficiency of powered systems for interproximal enamel reduction (IER) and enamel roughness before and after polishing—an in vitro study

Sebastian Zingler<sup>1</sup> · Andreas Sommer<sup>1</sup> · Sinan Sen<sup>1</sup> · Daniel Saure<sup>2</sup> · Jochen Langer<sup>3,4</sup> · Olivier Guillon<sup>3,5</sup> · Christopher J. Lux<sup>1</sup>

Published online: 24 May 2016  
© Springer-Verlag Berlin Heidelberg 2016

## Erratum to: Clinical Oral Investigations DOI 10.1007/s00784-015-1585-2

Accidentally Fig. 5 was shown twice (as Fig. 4 and Fig. 5) in the original version of the article. The correct version of Fig. 4 is shown below.

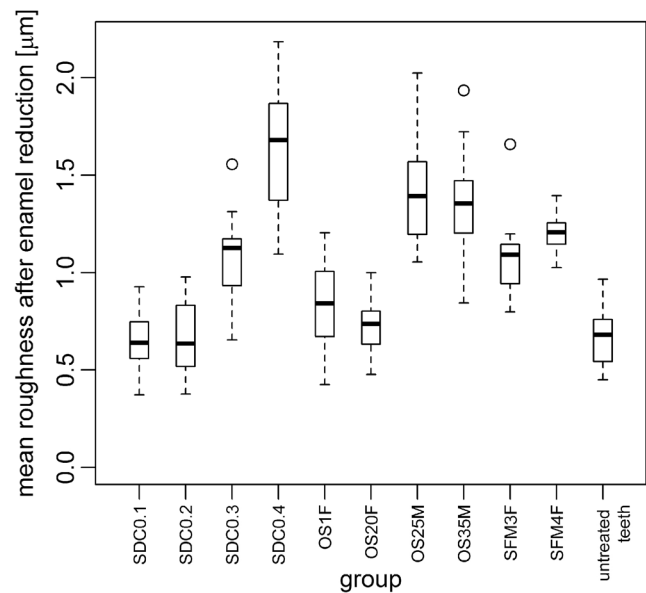

The online version of the original article can be found at <http://dx.doi.org/10.1007/s00784-015-1585-2>.

✉ Sebastian Zingler  
sebastian.zingler@med.uni-heidelberg.de

<sup>1</sup> Department of Orthodontics and Dentofacial Orthopaedics, University of Heidelberg, Heidelberg, Germany

<sup>2</sup> Institute of Medical Biometry and Informatics, University of Heidelberg, Heidelberg, Germany

<sup>3</sup> Institute of Materials Science, Technische Universität Darmstadt, Darmstadt, Germany

<sup>4</sup> Present address: Heraeus Holding GmbH, Hanau, Germany

<sup>5</sup> Present address: Forschungszentrum Jülich GmbH, Institute of Energy and Climate Research, Materials Synthesis and Processing, Jülich, Germany