

---

## CAN PHOTOPLETHYSMOGRAPHY VARIABILITY SERVE AS AN ALTERNATIVE APPROACH TO OBTAIN HEART RATE VARIABILITY INFORMATION?

Sheng Lu, PhD<sup>1</sup>, He Zhao, MS<sup>1</sup>, Kihwan Ju, PhD<sup>1</sup>,  
Kunsoo Shin, PhD<sup>2</sup>, Myounggho Lee, PhD<sup>3</sup>,  
Kirk Shelley, PhD<sup>4</sup> and Ki H. Chon, PhD<sup>1</sup>

---

From the <sup>1</sup>Department of Biomedical Engineering, State University of New York, SUNY@ Stony Brook HSC T18, Rm. 030, Stony Brook, NY, 11794-8181, USA; <sup>2</sup>Samsung Advanced Institute of Technology, Yongin-Si, South Korea; <sup>3</sup>Department of Electrical and Electronics Engineering, Yonsei University, Seoul, South Korea; <sup>4</sup>Department of Anesthesia, Yale University, New Haven, CT, USA.

Received 17 August 2007. Accepted for publication 24 October 2007.

Address correspondence to K. H. Chon, Department of Biomedical Engineering, State University of New York, SUNY@ Stony Brook HSC T18, Rm. 030, Stony Brook, NY, 11794-8181, USA.

E-mail: ki.chon@sunysb.edu

---

Lu S, Zhao H, Ju K, Shin KS, Lee MH, Shelley K, Chon KH. Can photoplethysmography variability serve as an alternative approach to obtain heart rate variability information?

J Clin Monit Comput 2008; 22:23–29

**ABSTRACT.** Heart rate variability (HRV), extracted from an electrocardiogram, is known to be a noninvasive indicator reflecting the dynamic interplay between perturbations to cardiovascular function and the dynamic response of the cardiovascular regulatory system. Photoplethysmography (PPG) is a noninvasive method to monitor arterial oxygen saturation on a continuous basis. Given the rich cardiovascular information in the PPG signal, and the ubiquity and simplicity of pulse oximetry, we are investigating the feasibility of acquiring dynamics pertaining to the autonomic nervous system from PPG waveforms. To do this, we are quantifying PPG variability (PPGV). Detailed algorithmic approaches for extracting accurate PPGV signals are presented. We compare PPGV to HRV by computing time and frequency domain parameters often associated with HRV measurements, as well as approximate entropy calculations. Our results demonstrate that the parameters of PPGV are highly correlated with the parameters of HRV. Thus, our results indicate that PPGV could be used as an alternative measurement of HRV.

**KEY WORDS.** autonomic nervous system, heart rate variability, pulse oximeter.

---

---

## INTRODUCTION

---

As a non-invasive means to monitor arterial oxygen saturation (SaO<sub>2</sub>) on a continuous basis, pulse oximetry is a well-established technology based on photoplethysmography that has become one of the most commonly used patient monitoring devices during anesthesia and in intensive care units. Given the ubiquity and simplicity of pulse oximetry, it is desirable to maximize its potential by exploring additional measurements we can derive from the pulse oximeter. In the present study, our goal was to determine if variations in the PPG signal can be used in lieu of heart rate variability (HRV) to extract dynamics pertaining to the autonomic nervous system.

HRV reflects the dynamic interplay between perturbations to cardiovascular function and the dynamic response of cardiovascular regulatory systems. It is clear from a work by Akselrod et al. [2] in the early 1980s, as well as numerous publications since, that maintaining ANS balance is important for cardiovascular health. Numerous studies have shown that altered variability in

the cardiovascular system is associated with a range of cardiovascular diseases and increased mortality [1, 9]. Cardiovascular variables such as heart rate, arterial blood pressure, and stroke volume, as well as lung volume, fluctuate on a beat-to-beat basis. The variability in cardiovascular signals reflects the homeostatic interplay between perturbations in cardiovascular functions and the dynamic responses of the cardiovascular regulatory systems [1, 6]. Thus, the normal heart rate is determined by many interacting systems, including the nervous system, baro- and chemoreceptors, local feedback loops in the heart, and several hormonal systems. These systems work on different time scales, and the complexity of this regulation is reflected in the apparently random fluctuations in heart rate [5]. There is considerable interest in these fluctuations because their simple statistical measures such as the standard deviation of the interbeat intervals (the  $R$ - $R$ -intervals), have been shown to be some of the strongest independent predictors of mortality after myocardial infarction [10]. Moreover, other techniques such as spectral analysis and nonlinear analysis of the  $R$ - $R$ -intervals of heart rate have been widely used in HRV studies, and on some occasions they have been shown to discriminate between subjects with different cardiac conditions as well as to predict mortality in some groups of patients [3, 9].

To date, only a few studies have demonstrated the use of PPG variability as a noninvasive measure of the dynamics pertaining to the autonomic nervous system, but none of these studies have provided detailed and direct quantitative comparison between the PPG and ECG signals [4, 11]. These studies were mainly based on the use of the pulse oximeter to examine specific cardiovascular problems that are associated with the autonomic nervous system. For example, one study has noted that in diabetic autonomic neuropathy patients, the rate of fall in percentage of oxygen saturation was significantly lower, less intense, and with delayed subsequent recovery compared to normal subjects [11]. In a separate study, recordings of the pulse oximeter waveforms during the Valsava maneuver were useful in rapid pre-operative identification of patients who have an autonomic neuropathy [4]. It is not surprising that only scant reports exist of using PPG variability as a noninvasive measure of the dynamics underlying the autonomic nervous system, since the rich information the pulse oximeter provides has only recently been appreciated. As the rise and fall of the PPG signal reflects the fluctuations of the heart beats, it is possible that PPG variability does reflect the dynamics of the autonomic nervous system. Our results show that this very hypothesis is feasible and that we can obtain similar information to that from HRV analysis. The significance

of using the PPG instead of the ECG is that this allows multi-functionality of the pulse oximetry, which would simplify many facets of monitoring systems, reduce healthcare costs, provide a more compact system, and the home health care monitoring more attainable.

---

## METHOD

---

Ten healthy subjects were involved in the study ( $26 \pm 7.47$  years). Twenty minutes (10 min in the upright position and 10 min in the supine position) of PPG waveform data (pulse oximeter module MP506, Nellcor Puritan Bennett) and ECG signal (HP 78354A patient monitor) were collected simultaneously and digitized with a sampling rate of 400 Hz (Powerlab 4SP, ADInstruments). HRV was obtained from ECG signals after  $R$ -wave peaks were detected, followed by cubic spline interpolation.

The PPG waveforms were denoised and detrended with empirical mode decomposition method (EMD) [12]. The EMD is based on a concept that any signal  $x(t)$  can be decomposed into a finite number of “intrinsic mode functions” (IMFs):

$$x(t) = \sum_{i=1}^n IMF_i + r_n$$

where  $r_n$  is a residue. An IMF is a function that satisfies two conditions:

- (1) The number of extrema and the number of zero crossings must either be equal or differ at most by one.
- (2) At any point the mean value of the envelope defined by the local maxima and the envelope defined by the local minima is zero.

IMFs represent oscillatory modes embedded within data where each IMF involves only one mode of oscillation. The EMD algorithm has been widely applied [7, 8], and thus, we only briefly summarize the following four steps:

- (1) Given the signal  $x(t)$ , identify the successive extrema of  $x(t)$ . Extract the upper and lower envelopes by interpolation and compute the average, and denote it as  $m_1$ :

$$m_1 = \frac{e_{\max}(t) + e_{\min}(t)}{2} \quad (1)$$

- (2) Subtract the envelope mean signal from the signal

$$h_1(t) = x(t) - m_1 \quad (2)$$

Treat  $h_1(t)$  as a new set of data, and repeat steps 1–2 until  $h_1(t)$  is converged. Then set  $C_1(t) = h_1(t)$ . The process stops when the difference between two consecutive shifts is smaller than a selected threshold SD, defined by

$$SD = \sum_{t=0}^T \left[ \frac{|h_{1(k-1)}(t) - h_{1k}(t)|^2}{h_{1(k-1)}^2(t)} \right] \quad (3)$$

- (3) Calculate the residue  $R_1(n) = x(n) - C_1(n)$ ; Treat  $R_1(n)$  as a new set of data, and repeat steps 1–2 until the residue becomes a constant or a monotonic function.
- (4)  $x(n) = C_1(n) + C_2(n) + \dots + C_N(n) + R_N(n)$ .  $C_i(n)$  is an intrinsic oscillatory mode and  $R_N(n)$  is the residue. Thus, the signal can be reconstructed by summing up all intrinsic oscillatory modes. When all the IMFs are extracted, the cross-correlation between each IMF and  $x(t)$  is calculated. The most correlated  $N$  number of IMFs whose dominant frequencies are larger than 0.5 Hz will be used to reconstruct the signal. In this way, most low frequency trends and high frequency noise can be removed. In our study, we used  $N = 4$ .

Once the low frequency trends and high frequency noise were removed via the EMD algorithm, the PPG variability series  $p$  was obtained by taking the first derivative of the down-slope phase of the PPG waveforms followed by selecting the resulting largest negative values. To ensure the robustness of the algorithm, two moving average processes were applied in the PPG variability detection procedure.

First, PPG waveforms are denoted as  $a(i)$ ,  $i = 1, 2, 3, \dots, N$  and the moving average of the signal  $a$  is performed:

$$b(i - M + 1) = \frac{1}{2M + 1} \sum_{j=i-M}^{i+M} a(j) \quad (4)$$

where  $i = M, M + 1, M + 2, \dots, N - M$  with  $M = fs/8$ . The  $fs$  refers to the sampling frequency. This ensures that the local minima of the PPG signals are accentuated when the derivative is taken in the proceeding step.

Second, define  $c$  as the successive difference (first derivative) series of  $b$ :

$$c(i) = \Delta b = b(i + 1) - b(i) \quad (5)$$

$$i = 1, 2, 3, \dots, N - 2M$$

Third, perform a second moving average of the signal  $c$ :

$$d(i - M + 1) = \frac{1}{2M + 1} \sum_{j=i-M}^{i+M} c(j) \quad (6)$$

where  $i = M, M + 1, M + 2, \dots, N - 3M$  with  $M = fs/8$ . Similar to the first moving average procedure, this facilitates choosing more accurate local minima.

Fourth, local minima and their positions are obtained by using an adaptive threshold ( $Th_a$ ) and a moving window length,  $W$ . Local minima obtained on the boundary of a moving window are neglected. Local minima should be no larger than the set adaptive threshold value. The length of a window should not exceed half of the cardiac cycle to avoid including down-slope segments from different cardiac cycles. In this study, the moving window length,  $W$ , was selected as  $fs/4 = 100$ . The adaptive threshold was obtained by setting  $Th_a(i) = ((i - 1\text{th}) \text{ local minimum})/3$ , where  $Th_a(1)$  is defined as the mean of the first 5 local minima, where  $i = 1, 2, 3, \dots, N$ . The moving average parameter  $M$  was selected as  $fs/8$ . Justification for this selection will be shown in the Results section.

To compare the similarity indices between PPGV and HRV, the following widely used time- and frequency-domain parameters are calculated and compared: the standard deviation of normal-to-normal  $R$ - $R$  intervals (SDNN), the root-mean square of the difference of successive  $R$ - $R$  intervals (RMSSD), the ratio of the low-to-high frequency spectra (LF/HF, LF: 0.04–0.15 Hz, HF: 0.15–0.4 Hz) and the approximate entropy (ApEn). ApEn is denoted as  $ApEn(m, r, N)$  where  $N$  is the length of the series to be analyzed and  $m$  determines the length of the sequences to be compared, which can be estimated by calculating the false nearest neighbor. The parameter  $r$  is the tolerance threshold for accepting similar patterns between two segments, and has been recommended to be within 0.1–0.2 times the standard deviation of the data [13].  $ApEn(m, r, N)$  is the average of the logarithms of the conditional probabilities that sequences of  $m$  beats which are “close” (within  $\pm r$ ) will remain “close” at the  $(m + 1)$ th beat:

$$ApEn = - \frac{\sum_{i=1}^{N-m} \ln \frac{C_i^{m+1}(r)}{C_i^m(r)}}{N - m} \quad (7)$$

where  $C_r^m(i) = V^m(i)/(N - m + 1)$  where  $V^m(i) = \text{no. of } d[X(i), X(j)] \leq r$ .

The student- $t$  test was used to determine whether there is a statistical significance between PPGV and HRV. Correlation coefficients were used to measure the linear relation between PPGV and HRV.  $p$ -values less than 0.05 were considered to be statistically significant.

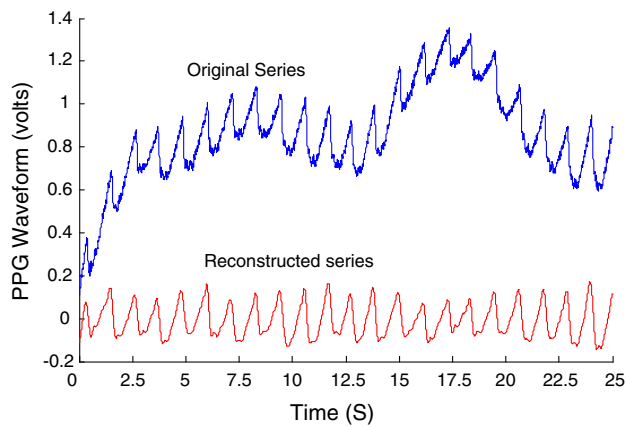


Fig. 1. Comparison of the original PPG and the reconstructed PPG waveforms based on the use of empirical mode decomposition.

**RESULTS**

A comparison between the original and the reconstructed PPG signal via the use of EMD is shown in Figure 1. The

reconstruction was based on using the four most correlated IMFs whose dominant frequency components are higher than 0.5 Hz. We note that both high and low frequency trends and noise are removed in the reconstructed signal. The EMD procedure was successful in removing noise and low frequency trends in all of the signals analyzed, and this procedure facilitates down-slope peak detection of the PPG waveforms.

Figure 2 shows a representative result obtained using the procedure outlined in the Methods section for the detection of the largest negative peak of the PPG waveform. Panel (a) is the detrended PPG waveform, panel (b) represents the moving average of the signal in panel (a), panel (c) represents the first derivative of the signal in panel (b), and panel (d) represents the moving average of the signal in panel (c). Details regarding the moving average and the derivative parameters are provided in the Methods section. The circles in panel (d) represent the position of the largest negative values. Note that as compared to panel (a), the negative values are better defined in panel (d). Finally, the PPGV signal is obtained by measuring the distance between two consecutive PPG signals in panel (d).

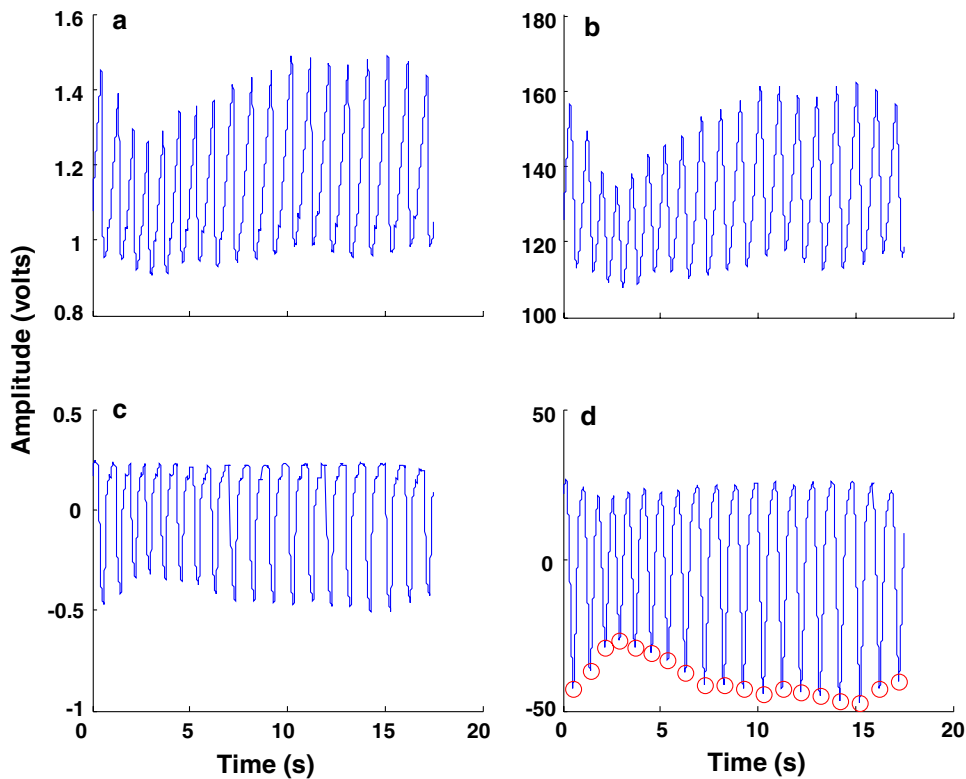


Fig. 2. Smoothing via moving average filter and the first derivative used to accentuate better detection of the local minima of the processed PPG signal. Panels a, b, c and d represent the PPG signal, moving average filter applied to the signal shown in panel a, derivative of the signal shown in panel b, and a second moving average filter on the signal shown in panel c, respectively.

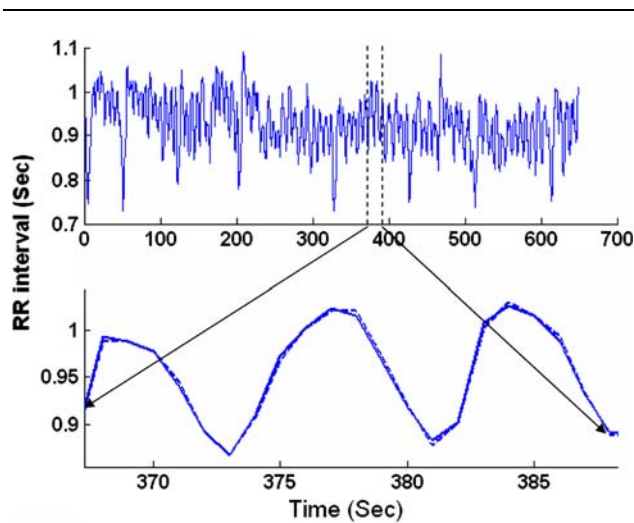


Fig. 3. Comparison of the HRV and PPG signals in the top panel shows that the signals are nearly identical. The bottom panel shows a segment of the upper panel, which further illustrates the closeness of the two signals.

The top panel of Figure 3 represents the overlap of the PPGV and HRV signals for a representative subject, and the bottom panel is a close-up one segment of PPGV (dotted line) and HRV (solid line) series. The solid and dotted lines match closely for all times, as Figure 3 shows. To quantitatively measure the similarity between the two signals, we computed the ratio between the power of the difference between PPGV and HRV to the power of HRV. The ratio is  $1.35 \pm 1.43\%$  for the supine position,  $3.03 \pm 2.78\%$  for the upright position, and the mean ratio between upright and supine is  $2.19 \pm 2.32\%$ . Thus, this is

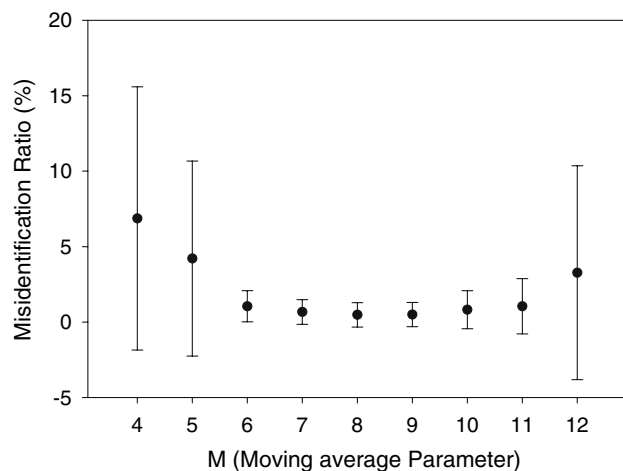


Fig. 4. Incorrect identification ratio of the PPG as a function of the size of the moving average parameter. Note that the incorrect identification ratio is relatively low when  $M$  is between  $f_s/6$  and  $f_s/9$ .

another indication that there is close similarity between the two signals.

As indicated in the Methods section, the selection of moving average parameter  $M$  is important to the accuracy of identifying the PPG variability time series. Figure 4 shows simulation results of the incorrect identification ratio of the PPGV as a function of the size of the moving average parameter. As shown, the incorrect identification ratio reaches the minimum of 0.54% when  $M = f_s/8$  but there is not much difference between  $M = f_s/6 - f_s/9$ .

Tables 1 and 2 show comparison of the HRV and PPGV derived time- and frequency-domain parameters consisting of SDNN, RMSSD, LF/HF and ApEn during supine and upright positions, respectively. As shown, there is no significant difference between parameters of PPGV and HRV for both supine and upright positions ( $p > 0.05$ ). Correlation coefficients between parameters of PPGV and HRV are shown in Tables 1 and 2, and they indicate strong correlation ( $p < 0.00001$ ) between parameters of PPGV and HRV, in all cases. We note that the correlation coefficients of parameters in the supine position are generally higher than those in the upright position, indicating that PPGV signals measured from the upright position are more affected by motion artifacts. List of abbreviations are provided in Table 3.

## DISCUSSION AND CONCLUSIONS

The promise of early detection and diagnosis of lethal cardiac arrhythmias based on noninvasive assessment of the autonomic nervous system via heart rate variability has led to significant interest among many researchers. In the biosignal processing field, the research focus is to develop more accurate algorithms that can be used for early diagnosis of malignant cardiac arrhythmias. In the field of cardiac monitoring systems, the current emphasis is on miniaturization of a system that is wireless and cost effective so that the measuring devices can be deployed to a large population. One such approach to accomplish the above-described three capabilities is to come up with a sensor that can extract many different physiological parameters, as the current environment is such that a sensor is limited to only one particular task. In this study, given the ubiquity and simplicity of the pulse oximeter, we investigate whether the PPGV can be used in lieu of heart rate variability to quantify and assess dynamic characteristics of the autonomic nervous system. If this is possible, then the pulse oximeter can have at least three different functionalities: blood oxygenation level, heart rate variability information, and respiratory rate. Having one sensor to perform all three tasks also facilitates compactness of the monitoring system facilitates making it

*Table 1. Quantitative comparison of the PPGV and HRV during supine position using linear time and frequency domain parameters as well as the nonlinear quantity ApEn. There were no statistical differences in all parameters shown, suggesting that the PPGV and HRV are similar*

Supine	SDNN (s)		RMSSD (s)		LF/HF (unitless)		ApEn (2,0.15) (unitless)	
	PPGV	HRV	PPGV	HRV	PPGV	HRV	PPGV	HRV
Sub 1	0.0641	0.0632	0.0426	0.0419	1.9061	1.9081	1.2005	1.1941
Sub 2	0.0574	0.0572	0.0371	0.0374	3.5228	3.3237	1.0262	1.0661
Sub 3	0.0524	0.0526	0.0383	0.0394	0.7316	0.6642	1.3854	1.4121
Sub 4	0.0368	0.0368	0.0311	0.0311	0.595	0.6772	1.3226	1.3153
Sub 5	0.0412	0.0404	0.0306	0.0293	1.4443	1.4595	0.9482	1.0095
Sub 6	0.0269	0.0251	0.0175	0.0144	0.2291	0.208	1.2257	1.323
Sub 7	0.0542	0.0519	0.0722	0.0679	0.9093	0.9485	1.009	1.0781
Sub 8	0.0633	0.062	0.0356	0.0347	0.3324	0.2684	1.2585	1.233
Sub 9	0.141	0.1405	0.149	0.1498	0.6884	0.6791	1.2554	1.2676
Sub 10	0.0207	0.0204	0.0118	0.0117	1.6075	1.7337	1.3844	1.3443
Student- <i>t</i> test, <i>p</i>	0.958		0.964		0.983		0.732	
$r^2$	0.9997*		0.999*		0.9964*		0.9649*	

wireless as it reduces the bandwidth as well as battery consumption, and reduces the cost significantly as it eliminates the need for having three separate sensors and their associated supporting hardware requirements.

The feasibility of the PPGV was verified by comparing both time and frequency-domain parameters of the HRV, which all demonstrated high correlation between the two signals. Likewise, ApEn values were not statistically

different for both signals. Our results were aided by our preprocessing procedures of the PPG data which involved elimination of low and high frequency trends as well as simple derivative and moving average procedures to accentuate the detection of local minima.

We observed that the PPG signal obtained during the upright position had more motion artifacts than during the supine position, as evidenced by a lower correlation

*Table 2. Quantitative comparison of the PPGV and HRV during upright position via linear time and frequency domain parameters as well as the nonlinear quantity ApEn. There were no statistical differences in all parameters shown, suggesting that the PPGV and HRV are similar*

Upright	SDNN (s)		RMSSD (s)		LF/HF (unitless)		ApEn (2,0.15) (unitless)	
	PPGV	HRV	PPGV	HRV	PPGV	HRV	PPGV	HRV
Sub 1	0.0327	0.0311	0.0132	0.0104	2.0875	2.9932	1.0722	1.1941
Sub 2	0.0588	0.0582	0.0229	0.0222	7.0911	7.5436	1.1471	1.0661
Sub 3	0.0491	0.048	0.0178	0.0157	8.3334	10.3396	0.9648	1.4121
Sub 4	0.0279	0.0271	0.0119	0.0097	1.4044	2.7836	1.2213	1.3153
Sub 5	0.0347	0.0327	0.0193	0.0173	3.0242	3.3079	0.9086	1.0095
Sub 6	0.0365	0.0365	0.0286	0.0289	1.3458	1.9998	1.1851	1.1851
Sub 7	0.0311	0.0279	0.0254	0.0195	1.0841	1.3121	1.4042	1.3689
Sub 8	0.0561	0.0541	0.0289	0.0269	1.2307	1.8484	1.0484	0.9925
Sub 9	0.0669	0.0642	0.0394	0.0374	0.5892	0.6656	1.1899	1.1809
Sub 10	0.0232	0.0225	0.0109	0.0079	6.2982	12.4375	1.1184	0.9953
Student- <i>t</i> test, <i>p</i>	0.827		0.594		0.431		0.569	
$r^2$	0.9977*		0.9858*		0.9254*		0.967*	

Table 3. List of abbreviations

ApEn	Approximate Entropy
ECG	Electrocardiogram
EMD	Empirical Mode Decomposition
HF	High Frequency
HRV	Heart Rate Variability
IMF	Intrinsic Mode Function
LF	Low Frequency
PPG	Photoplethysmography
PPGV	Photoplethysmography Variability
RMSSD	Root-mean Square of the Successive Difference
SDNN	Standard Deviation of Normal-to-Normal

between the HRV and PPGV signals. In addition, unless an adaptive filtering scheme such as Wiener filtering is used, the PPG signal is susceptible to significant motion artifacts which even the EMD has difficulty in eliminating. Thus, future studies need to address elimination of significant motion artifacts in the PPG signal in situations where they are unavoidable. However, given the fact that pulse oximetry is ubiquitous, simple to use and has the potential to provide multi-physiological parameters, its advantages outweigh the current shortcomings. The current work strongly suggests a good alternative to understanding dynamics pertaining to the autonomic nervous system without the use of an ECG device. Most importantly, the multi-functional pulse oximeter-based device has the tremendous potential to be readily accepted by patients due to its simplicity and comfort, not to mention the significant potential to decrease health care costs as compared to the current practice of using multiple sensors and devices to obtain the data.

## REFERENCES

1. Heart rate variability: standards of measurement, physiological interpretation and clinical use. Task force of the European society of cardiology and the north american society of pacing and electrophysiology. *Circulation* 1996; 93: 1043–1065.
2. Akselrod S, Gordon D, Madwed JB, Snidman NC, Shannon DC, Cohen RJ. Hemodynamic regulation: investigation by spectral analysis. *Am J Physiol* 1985; 249: H867–H875.
3. Bigger JT Jr., Fleiss JL, Rolnitzky LM, Steinman RC, Schneider WJ. Time course of recovery of heart period variability after myocardial infarction. *J Am Coll Cardiol* 1991; 18: 1643–1649.
4. Broome IJ, Mason RA. Identification of autonomic dysfunction with a pulse oximeter. *Anaesthesia* 1988; 43: 833–836.
5. Davies CT, Neilson JM. Sinus arrhythmia in man at rest. *J Appl Physiol* 1967; 22: 947–955.
6. Eckberg DL. Sympathovagal balance: a critical appraisal. *Circulation* 1997; 96: 3224–3232.
7. Huang W, Shen Z, Huang NE, Fung YC. Engineering analysis of biological variables: an example of blood pressure over 1 day. *Proc Natl Acad Sci U S A* 1998; 95: 4816–4821.
8. Huang W, Shen Z, Huang NE, Fung YC. Use of intrinsic modes in biology: examples of indicial response of pulmonary blood pressure to +/- step hypoxia. *Proc Natl Acad Sci USA* 1998; 95: 12766–12771.
9. Huikuri HV, Koistinen MJ, Yli-Mayry S, Airaksinen KE, Seppanen T, Ikaheimo MJ, Myerburg RJ. Impaired low-frequency oscillations of heart rate in patients with prior acute myocardial infarction and life-threatening arrhythmias. *Am J Cardiol* 1995; 76: 56–60.
10. Kleiger RE, Miller JP, Bigger JT Jr., Moss AJ. Decreased heart rate variability and its association with increased mortality after acute myocardial infarction. *Am J Cardiol* 1987; 59: 256–262.
11. Modi KD, Sharma AK, Mishra SK, Mithal A. Pulse oximetry for the assessment of autonomic neuropathy in diabetic patients. *J Diabetes Complications* 1997; 11: 35–39.
12. Huang NE, SRL, Shen Z. The mechanism for frequency downshift in nonlinear wave evolution. *Adv Appl Mech* 1996; 32: 59–111.
13. Pincus SM. Approximate entropy as a measure of system complexity. *Proc Natl Acad Sci USA* 1991; 88: 2297–2301.