

ARTICLE

Received 4 Apr 2015 | Accepted 13 Aug 2015 | Published 14 Oct 2015

DOI: 10.1038/ncomms9345

OPEN

Accurate lineshape spectroscopy and the Boltzmann constant

G.-W. Truong^{1,2}, J.D. Anstie^{1,2}, E.F. May³, T.M. Stace⁴ & A.N. Luiten^{1,2}

Spectroscopy has an illustrious history delivering serendipitous discoveries and providing a stringent testbed for new physical predictions, including applications from trace materials detection, to understanding the atmospheres of stars and planets, and even constraining cosmological models. Reaching fundamental-noise limits permits optimal extraction of spectroscopic information from an absorption measurement. Here, we demonstrate a quantum-limited spectrometer that delivers high-precision measurements of the absorption lineshape. These measurements yield a very accurate measurement of the excited-state ($6P_{1/2}$) hyperfine splitting in Cs, and reveals a breakdown in the well-known Voigt spectral profile. We develop a theoretical model that accounts for this breakdown, explaining the observations to within the shot-noise limit. Our model enables us to infer the thermal velocity dispersion of the Cs vapour with an uncertainty of 35 p.p.m. within an hour. This allows us to determine a value for Boltzmann's constant with a precision of 6 p.p.m., and an uncertainty of 71 p.p.m.

¹Institute for Photonics and Advanced Sensing (IPAS) and School of Chemistry and Physics, The University of Adelaide, Adelaide, South Australia 5005, Australia. ²School of Physics, The University of Western Australia, Perth, Western Australia 6009, Australia. ³Centre for Energy, School of Mechanical and Chemical Engineering, The University of Western Australia, Crawley, Western Australia 6009, Australia. ⁴ARC Centre for Engineered Quantum Systems, University of Queensland, Brisbane 4072, Australia. Correspondence and requests for materials should be addressed to G.-W.T (email: gar-wing.truong@uwa.edu.au) or to T.M.S. (email: stace@physics.uq.edu.au) or to A.N.L. (email: andre.luiten@adelaide.edu.au).

Spectroscopy is a vital tool for both fundamental and applied studies. Improving both the precision and accuracy of spectroscopic measurements is critical to efforts targeted at gaining maximum physical information about the quantum absorbers—even as they are perturbed by the probe. The immediate motivation for our work has arisen out of a call to the scientific community to develop new techniques to re-measure Boltzmann's constant, k_B , in preparation for a redefinition of the kelvin¹; however, advances in absorption lineshape measurement and theory will find applications in accurate gas detection and monitoring², studies of planetary atmospheres³, thermometry in tokamaks⁴ and understanding distant astrophysical processes^{5,6}. The accurate measurement of natural linewidths and transition frequencies, which can be directly related to the atomic lifetime, level structure and transition probabilities, is important for testing atomic physics^{7–9}.

At thermal equilibrium, the velocity distribution of atomic absorbers in a vapour cell is related to the temperature through the Boltzmann distribution. This simple and fundamental relationship forms an excellent foundation for a type of primary thermometry known as Doppler broadening thermometry (DBT)^{10,11}. DBT differs from the current leading technique for primary thermometry, which measures the temperature-dependent speed of sound in a noble gas contained in a well-characterized acoustic resonator. Using that approach, a breakthrough determination of k_B was made in 1988 with a total uncertainty of 1.7 p.p.m. (ref. 12). Refinements to this technique over the last 20 years have reduced its uncertainty to the 1 p.p.m. level^{13,14}, improving the uncertainty in the CODATA-recommended value for k_B from 1.8 p.p.m. (CODATA-02) to 0.91 p.p.m. (CODATA-10). Despite these superb measurements, it is important that different techniques are employed to measure k_B to reduce the possibility of underestimating systematic uncertainties that may be inherent to any single technique¹⁵.

The DBT approach is one of the most theoretically transparent of the new approaches to primary thermometry. The spectrum of a gas sample is measured with high precision, and a theoretical model is fitted to the measured data. If the model includes all of the relevant physics then one can accurately extract the contribution to spectral broadening arising solely from the thermal distribution of atomic/molecular speeds. Ammonia probed by a frequency-stabilized CO₂ laser at 1.34 μm was the first thermometric substance employed in a DBT experiment¹⁶. Subsequently, an extended-cavity diode laser at 2 μm was used to probe a ro-vibrational transition of CO₂ (ref. 17). In these first experiments, the lineshape was assumed to be a Gaussian or a Voigt profile (a Gaussian convolved with a Lorentzian). Since 2007, with the ambitious goal of approaching 1 p.p.m. accuracy, substantial experimental and theoretical improvements have been made to DBT using ammonia^{18,19}, oxygen²⁰, ethyne²¹ and water²². However, one key challenge peculiar to molecular absorbers is the need to account for complex collisional effects on the lineshape¹⁹. We avoid this by using a dilute atomic vapour^{23,24} with a strong dipole transition for which a tractable, microscopic theory has been developed^{25,26}. The benefits of a range of different atomic species have been considered in ref. 27.

Here we present measurements of a transmission lineshape of cesium (Cs) vapour with a quantum-limited transmission uncertainty of 2 p.p.m. in a 1 s measurement, which is to our knowledge, a factor of 16 times superior to anything previously demonstrated²⁸. This extreme precision, allows us to directly detect subtle lineshape perturbations that have not been previously observed. This observation prompted the development of a theoretical model, which now allows us to discriminate between the internal atomic state dynamics and their external motional degrees. Using the model we are able to estimate the

velocity dispersion of the atoms with a precision (s.e.) of 53 p.p.m. during a single-line scan, taking ~ 30 s. This is consistent with the sample s.d. (also 53 p.p.m.) over multiple scans, demonstrating the excellent reproducibility of the spectrometer. The measurement precision averages down to 3.7 p.p.m. after 200 scans. These values are ~ 7 times better than the previous best results^{28–30}, and also yields a near-two-fold reduction in the uncertainty of the excited-state hyperfine splitting in Cs³¹. Our measurement of the homogenous broadening component of the lineshape has a precision within a factor of two of the best ever measurements of natural linewidth. Modest improvements in the probe laser performance would deliver a new result for the excited state lifetime of Cs in a system that is experimentally and theoretically much simpler than that typically used for lifetime studies^{32,33}.

Results

Transmission spectra. We measure the transmission through the vapour cell as the probe laser frequency scans across the Cs D1 transition ($6S_{1/2}$ – $6P_{1/2}$), shown in Fig. 1a. The relative noise in the measurement of the atomic transmission is set by the shot noise in the probe and reference beams, and provides 2 p.p.m. in a 1 s measurement (at the highest optical powers used). The two absorption dips seen in Fig. 1a come from the hyperfine splitting in the excited state and the excellent signal-to-noise ratio enables

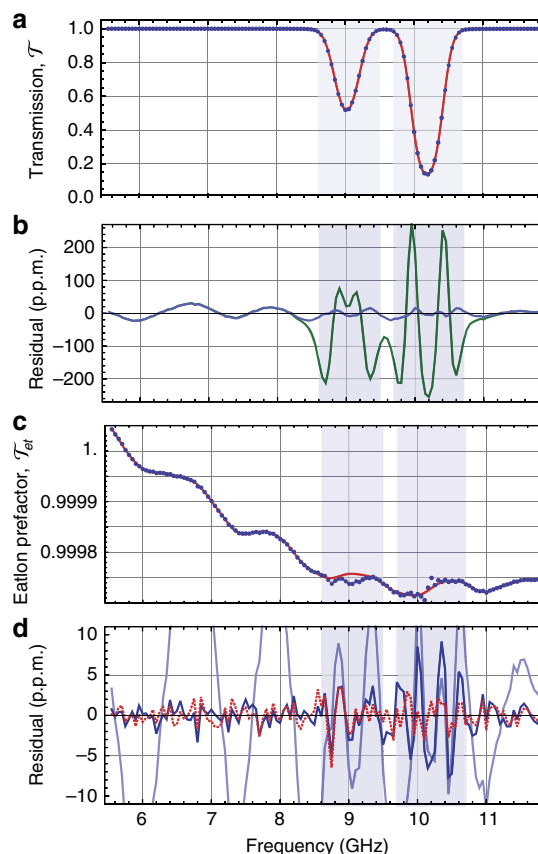


Figure 1 | Typical transmission spectra and fit residuals. (a) Measured transmission at 296 K for the highest intensity, $I/I_{\text{sat}} = 0.0028$, averaged over 200 scans (points) and theory (solid). (b) Residuals including Voigt-only (dark green) and first-order correction (light blue). (c) Etalon pre-factor, equation (1), with 6 etalons (solid) and data divided by second-order power-corrected Voigt profiles (points), assuming $\Gamma_L = 2.327$ MHz. (d) Residuals after including first-order correction with 0 etalons (light blue) and 6 etalons (dark blue), and second-order with 6 etalons (dotted red).

us to determine this splitting to be $f_{\text{HFS}} = 1167.716(3)$ MHz. The accuracy of this measurement exceeds that of the previous best determination³¹ in which a sub-Doppler atomic beam spectroscopy technique was used to measure f_{HFS} . Spectroscopy in vapour cells is appealing for its ease of implementation, but as Gerginov *et al.* identified, such approaches often suffer from optical-pumping-related systematics that necessarily arise in the creation of sub-Doppler absorption features. Here, we avoid this by greatly improving the detection sensitivity and perturbatively accounting for non-linear absorption effects in our lineshape model.

The conventional description of an absorption lineshape, $T_{\text{at}}(f)$, of an atomic transition with a rest-frame transition frequency f_0 , is given by a convolution of a Lorentzian function with a natural (half) linewidth $\Gamma_L = 1/(4\pi\tau)$ due to the finite lifetime τ of the transition, with a Gaussian distribution having a e^{-1} -width $\Gamma_D = f_0\sqrt{2k_B T/(m_Cs c^2)}$ due to Doppler broadening of atoms of mass m at temperature T . By fitting a lineshape to the measured transmission data, with Γ_D^{fit} as a fitting parameter, we extract the Doppler component, from which we infer the temperature. Systematic errors in Γ_D^{fit} are quantified by converting the independent PRT temperature measurements into an expected Doppler width, Γ_D^{PRT} , using the CODATA values for k_B and m_{Cs} , which we compare with Γ_D^{fit} .

If the natural lineshape of the transition is a Lorentzian, then the resulting convolution is the well-known Voigt profile, which is commonly used to model dipole resonances. However, our extremely low-noise transmission measurements reveal deviations from the Voigt profile. Some of these deviations are technical in origin for example, instrumental broadening due to the lineshape of the probing laser, residual spontaneous emission from the probe laser, unwanted optical etalons and photodetector linearity; however, there is an important fundamental effect resulting from frequency-dependent optical pumping, which perturbs the atomic natural lineshape away from a Lorentzian. All of these effects, whether technical or fundamental, cause systematic perturbations to the lineshape, and must be taken into account to model the lineshape accurately.

Least-squares fitting. To demonstrate these deviations, we fit a model consisting of two Voigt profiles separated by f_{HFS} , to the raw transmission data shown Fig. 1a. The residuals of this Voigt-only fit have characteristic ‘M’-shaped features near resonance, with amplitude ~ 200 p.p.m. at the highest probe powers, as shown in the green trace in Fig. 1b. These features demonstrate the breakdown of the Voigt profile, indicating additional, unaccounted for physics, which causes a spurious linear dependence of Γ_D^{fit} on probe intensity, as shown in the green curve in Fig. 2. In what follows, we describe how we sequentially include additional physics in our transmission model to remove these, and other, systematic effects, leaving only the shot-noise limit of our detection apparatus.

In earlier work we showed that the ‘M’-shaped features in Fig. 1b arise from atomic population dynamics induced by the probe laser, which are significant even at exceedingly low intensities²⁵. We subsequently calculated corrections to the Voigt profile up to linear order in the probe intensity²⁶, to account for optical pumping. Including this first-order intensity-dependent corrections in our model suppresses the features substantially, as shown in the blue trace in Fig. 1b.

Treatment of etalons. Far from the resonances, oscillations are evident in the residuals shown in Fig. 1b, which are clearly resolved due to our very high transmission measurement

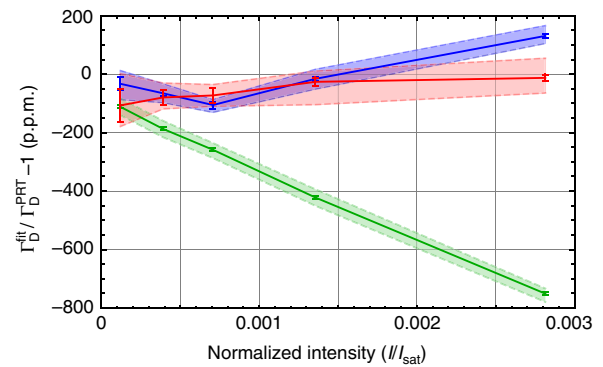


Figure 2 | Power dependence of the fitted Doppler width. Fractional deviation between the fitted Doppler width and that inferred from PRT temperature are plotted for measurements at 296 K. Green points are fits using the conventional Voigt-only profile. Blue points are fits using the first-order intensity-dependent correction. Red points are fits using the second-order intensity-dependent correction. Solid curves are fits using our central estimate of $\bar{\Gamma}_L = 2.327$ MHz; dashed curves are for $\bar{\Gamma}_L = 2.320$ MHz (upper) and $\bar{\Gamma}_L = 2.334$ MHz (lower) representing $\bar{\Gamma}_L \pm \sigma_{\bar{\Gamma}_L}$; the shaded regions indicate the sensitivity of Γ_D^{fit} to Γ_L in this range. Error bars represent s.e. of fits to the average of 200 scans for fixed Γ_L .

sensitivity (see also ref. 17). These oscillations arise from low-finesse etalons in the optics used to deliver the light to the atoms. An alternate thesis, that these features might arise from photoassociation of Cs atoms, can be discarded as these effects can be shown to be immeasurable at the present number density (see the Error Budget section of the Supplementary Discussion and ref. 34). Etalons are of particular concern for DBT since they introduce systematic errors in Γ_D^{fit} . In the Etalon Reduction section of the Supplementary Methods, we show that scattered light at the level of 0.1 p.p.b. of the beam power from non-reflecting surfaces can produce etalons with amplitude 30 p.p.m., consistent with the dominant etalon seen in Fig. 1b. Although obviously technical in nature, reducing the etalons beyond this already small amplitude is an experimental challenge. To handle these residual etalons in the analysis, we include etalons in our transmission model so that the total transmission is given by $T = T_{\text{at}}\mathcal{T}_{\text{et}}$, where \mathcal{T}_{et} includes N_{et} etalons and a slowly varying quadratic background:

$$\mathcal{T}_{\text{et}}(f) = \frac{\alpha + \beta f + \gamma f^2}{\prod_{j=1}^{N_{\text{et}}} \left(1 + a_j \sin^2\left(\pi f/f_j + \phi_j\right)\right)}, \quad (1)$$

where f_j is the free-spectral range of etalon j .

We add etalons to the model until the residuals far from resonance are consistent with a white-noise background. For completeness, we can include up to $N_{\text{et}} = 6$ etalons, with the smallest resolved etalons having amplitude of a few p.p.m. The solid curve in Fig. 1c shows \mathcal{T}_{et} for the highest power data; the points show the raw transmission data divided by the fitted T_{at} , demonstrating that \mathcal{T}_{et} is uncorrelated with the atomic transmission profile shown in Fig. 1a. The Etalon Reduction section of the Supplementary Methods has a detailed analysis of etalon fitting, showing that it is robust, and with $N_{\text{et}} \geq 2$ etalons we recover a stable value of Γ_D^{fit} .

Optical pumping perturbations. The dark-blue trace in Fig. 1d includes first-order power-dependent corrections, and 6 etalons. Away from resonance, the residuals are then consistent with the noise floor of our apparatus. However, around the deepest resonance we observe ~ 10 p.p.m. features. To eliminate these

Table 1 | Error budget for the determination of the Boltzmann constant at 296 K.

Source	$u_r(k_B)$ (p.p.m.)
Statistical (from Fig. 3)	5.8
Lorentz width (Γ_L^{fit})*	65
Lorentz width (Γ_L^{ind})†	190
Laser Gaussian noise	16
Optical pumping	15
Etalons (misidentification)	15
Etalons (unresolved)	3
Spontaneous emission	3.6
Temperature	1.9
Temperature gradient	1.2
PD linearity	1
Zeeman splitting	<1
Atomic recoil	<1
Photoassociation	<1
Quantum interference	0
Total (fit Γ_L)	71
Total (independent Γ_L)	191

Optical pumping shifts are reported at $I/I_{\text{sat}} = 3 \times 10^{-3}$ assuming second-order corrections to the Voigt profile. u_r denotes fractional uncertainty.
*Estimated from fits to scan data with free Lorentz width.
†Estimated from published uncertainty in Cs lifetime, plus uncertainty in the independent estimate of the laser linewidth.

we include second-order intensity-dependent corrections to the Voigt profile of each resonance (see the Lineshape Corrections at Second Order in Intensity section in the Supplementary Discussion):

$$T_{\text{at}} = e^{-pV_v(\Delta)} \left(1 + q_1 \left(e^{-pV_v(\Delta)} - 1 \right) V_v^{(2)}(\Delta) / V_v(\Delta) \right. \\ \left. + q_2 \left(\left(e^{-pV_v(\Delta)} - 1 \right) V_v^{(2)}(\Delta) / V_v(\Delta) \right)^2 \right. \\ \left. + q_3 \left(e^{-2pV_v(\Delta)} - 1 \right) V_v^{(3)}(\Delta) / V_v(\Delta) \right), \quad (2)$$

where $v = \Gamma_D / \Gamma_L$, Δ is the detuning from the resonance, and the generalized Voigt profile is given by $V_v^{(n)}(\Delta) = \pi^{-3/2} \int_{-\infty}^{\infty} dx e^{-(\Delta-x)^2/v^2} (1+x^2)^{-n}$, and the conventional Voigt profile is $V_v(\Delta) = V_v^{(1)}(\Delta)$. For a cell of length L with linear absorption coefficient α , the optical depth on resonance is $p = \alpha L$, $q_1 \propto I$ is the linear intensity-dependent coefficient²⁵, and $q_{2,3} \propto I^2$ are quadratic intensity-dependent coefficients.

The red-dotted trace in Fig. 1d shows the residuals after including second-order intensity corrections. The residuals are suppressed to ~ 2 p.p.m., consistent with the detection noise floor, giving confidence that the transmission model accounts for systematic effects.

Figure 2 compares the fractional deviation between Γ_D^{fit} and Γ_D^{PRT} as a function of incident intensity for the three possible models for the atomic lineshape: Voigt-only (green), first-order (blue) and second-order (red) intensity-dependent corrections. Naturally, the true Γ_D should be intensity independent. The simplest Voigt-only theory clearly exhibits a linear intensity dependence, leading to ~ 750 p.p.m. discrepancy even at intensities as low as $I/I_{\text{sat}} = 2.8 \times 10^{-3}$ where $I_{\text{sat}} = 2.5 \text{ mW cm}^{-2}$ is the saturation intensity for the transition³⁵. From ref. 26, we expect the first-order correction to have a residual quadratic dependence on intensity, which is consistent with the blue curve on Fig. 2. Finally, the second-order correction (red curve) is seen to suppress all intensity dependence to below the measurement precision. The simultaneous removal of all systematic features from the residuals together with the

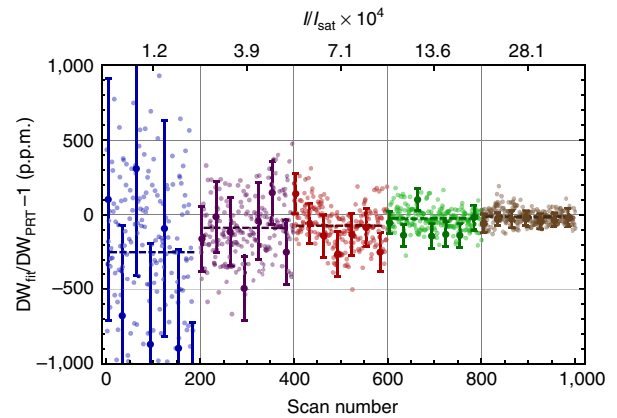


Figure 3 | Scatter of Doppler width determinations. The deviation between Γ_D^{fit} (using second-order intensity correction with $\Gamma_L = 2.327$ MHz) and Γ_D^{PRT} are plotted, for each scan at 296 K. Colours and vertical gridlines demark different incident intensities (as shown along top axis), corresponding to normalized intensities in Fig. 2. Dashed lines are the mean of the corresponding set of scans, error bars are the estimated parameter error ($\pm 1\sigma$) for each selected scan, and are consistent with sample s.d. Etalons are included in each fit, with parameters fixed by fits to the average of all scans within a power level, that is, etalon parameters are not free to vary within a particular power level.

elimination of intensity dependence in the recovered Γ_D^{fit} gives a high degree of confidence that the model includes all relevant physics.

We note briefly that in fluorescence spectroscopy one should account for quantum interference between different hyperfine manifolds^{36–40}. This is not an issue in absorption spectroscopy (see the Quantum Interference section of the Supplementary Discussion).

Application to primary thermometry. In this section we demonstrate the power of our spectroscopic technique by applying it to the problem of primary thermometry, and determine a value for Boltzmann's constant using atomic spectroscopy.

The atomic vapour is thermalized at around $T = 296$ K (that is, $\Gamma_D^{\text{PRT}} = 215.123$ MHz) by suspending it in a thermal isolator. The independent PRT measurement has an uncertainty of 0.55 mK (1.9 p.p.m.). We note the temperature drifted over the course of the experimental scans, such that Γ_D^{PRT} is expected to vary from ~ 214.96 to 215.13 MHz (see Supplementary Fig. 7).

After systematically removing the effects of optical pumping and etalons, the largest source of uncertainty in Γ_D^{fit} comes from the uncertainty in Γ_L . We obtain a value for Γ_L by directly fitting it to the data, which gives $\Gamma_L^{\text{fit}} = 2.327(7)$ MHz. This is consistent with, but also more precise than, an independent estimate, $\Gamma_L^{\text{ind}} = 2.331(19)$ MHz, given by the sum of the natural linewidth of the Cs $6P_{1/2}$ level, $\Gamma_L^{\text{at}} = 2.287(6)$ MHz (ref. 35), and the laser linewidth, $\Gamma_L^{\text{las}} = 0.044(18)$ MHz. From Fig. 2 we estimate that a 1 kHz change in Γ_L leads to ~ 5 p.p.m. change in Γ_D^{fit} , so that the 6.5 kHz uncertainty in Γ_L contributes 32.5 p.p.m. uncertainty in Γ_D^{fit} (65 p.p.m. in $u_r(k_B)$). We note that if the probe linewidth were ~ 1 kHz, then our measurement would yield a state-of-the-art value for the excited-state lifetime of Cs.

We now briefly describe additional sources of uncertainty, which are quantified in Table 1 (see the Error Budget section of the Supplementary Discussion for a comprehensive description). Statistical error arising from the scatter in Fig. 3 contributes 2.9 p.p.m. to $u_r(\Gamma_D^{\text{fit}})$ (5.8 p.p.m. to $u_r(k_B)$). This is also consistent

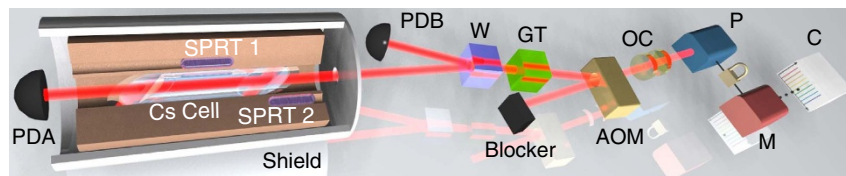


Figure 4 | High-accuracy linear absorption spectrometer for probing the D1 transitions in atomic Cs vapour. A probe laser (P) is offset-frequency locked to a master laser (M), which is in turn compared against a stabilized optical frequency comb (C). The probe laser output is spectrally and spatially filtered with an optical cavity (OC) before being deflected by an acousto-optic modulator (AOM). The beam is then passed through a Glan-Taylor (GT) prism and divided on a Wollaston (W) beam splitter. The power of the beam transmitted through the Cs cell inside the thermal and magnetic shield is measured on a photodetector PDA and compared with a reference beam measured on photodetector PDB. SPRT1 and SPRT2 are standard platinum resistance thermometers from which we independently measure the cell temperature.

with the estimated s.e. for each point in Fig. 3, shown as error bars. The probe laser has a Gaussian noise component causing 0.88(39) MHz of broadening contributing 8 p.p.m. to $u_r(\Gamma_D^{\text{fit}})$ (16 p.p.m. to $u_r(k_B)$). Residual effects of optical pumping after second-order power corrections contribute 7.5 p.p.m. to $u_r(\Gamma_D^{\text{fit}})$ (15 p.p.m. to $u_r(k_B)$). Misidentification of etalon parameters contributes 7.5 p.p.m. to $u_r(\Gamma_D^{\text{fit}})$ (15 p.p.m. to $u_r(k_B)$). Possible unresolved etalons contribute 3 p.p.m. to $u_r(k_B)$. Residual spontaneous emission from the laser, after filtering by the optical cavity, contributes 3.6 p.p.m. to $u_r(k_B)$. In the Error Budget section of the Supplementary Discussion, we calculated the effects of atomic recoil caused by the probe beam itself and quantum interference between the two atomic resonances and found them to be negligible.

To determine a value for k_B , we take a weighted mean of $\Gamma_D^{\text{fit}}/\Gamma_D^{\text{PRT}}$ extracted from fits using all the second-order corrected data shown on Fig. 2 (red points). We find $k_B = 1.380545(98) \times 10^{-23} \text{ J K}^{-1}$, where the 71 p.p.m. uncertainty is calculated in Table 1. This is consistent with the recommended CODATA value of $1.3806488(13) \times 10^{-23} \text{ J K}^{-1}$.

Discussion

In conclusion, we have developed an atomic absorption spectrometer that operates with a transmission measurement precision of just 2 p.p.m. This has revealed several new phenomena. Combined with a perturbative treatment of optical pumping we are able to explain all of the observed effects to a level of precision never before demonstrated. The power of our technique is demonstrated by measuring the lineshape parameters of thermal vapour. The reproducibility is consistent with the quantum limits of measurement⁴¹ giving confidence that we have captured the relevant physics.

With this unprecedented sensitivity, we have measured the transmission spectrum of Cs at 895 nm at the laser intensity shot-noise limit. From these spectra, we derive a value for Boltzmann's constant with an uncertainty of 71 p.p.m., consistent with the recommended CODATA value, and the hyperfine frequency splitting of the $6^2P_{1/2}$ level with the lowest uncertainty ever previously reported:

$$k_B = 1.380545(98) \times 10^{-23} \text{ J/K} \quad (3)$$

$$f_{\text{HFS}} = 1167.716(3) \text{ MHz.} \quad (4)$$

Statistical uncertainty contributes 6 p.p.m. to our error budget, after averaging spectra taken over a few hours of data acquisition. Our total uncertainty is dominated by imprecision in the literature value of the excited state lifetime of the Cs D1 transition (known to 0.26% (ref. 35)).

Although drifts in the experiment are likely in the apparatus on timescales required for multiple scans (for example, in the absolute optical frequency of the master laser), we average only the fitted parameters from each spectrum that are insensitive to

the drifts; for example, the centre frequency of each resonance cannot be determined to a better accuracy than the stability of the master laser, but their difference can be averaged over long timescales to achieve a lower uncertainty.

A future experiment designed to further minimize etalons, and using a higher power, sub-kHz linewidth probe laser with greater tuning range ($\sim 30 \text{ GHz}$) would eliminate probe laser effects, allow better estimation of etalon contamination, and lower the contribution of optical pumping. This opens the door to the best measurement of the Cs D1 transition lifetime, and a p.p.m.-level measurement of k_B thus making an important contribution to efforts to redefine the kelvin.

Methods

Probe light preparation. The spectrometer is pictured in Fig. 4a. The probe laser (P) is tightly locked at a tunable frequency difference away from a master laser (M), which is itself stabilized to an atomic transition in Cs. The frequency stability of the master laser is compared with a reference frequency provided by an optical frequency comb (C). The probe laser is spectrally and spatially filtered using a combination of an optical cavity (OC) of moderate finesse ($\mathcal{F} \approx 305$) and single-mode fibre (not shown). This reduces the spontaneous emission content of the probe beam from 1.6% to below 0.01%. The optical power is actively stabilized with an acousto-optic modulator (AOM). It is then delivered into a vacuum chamber in which the vapour cell is mounted in a thermal and magnetic shield. Calibrated standard platinum resistance thermometers (SPRTs) were used to independently measure the temperature of the shield and control it with a precision of a few millikelvin. Spatial temperature gradients are suppressed to the same level.

Measurement scheme. Inside the vacuum chamber, the probe light is split into two beams using a combination of a Glan-Taylor polarizing prism (GT) and Wollaston beam splitter (W). One beam passes through a Cs cell embedded inside the thermal and magnetic shield and is measured by photodiode A (PD A); the other beam is measured directly by photodiode B (PD B). The ratio of these photodiode signals gives us the transmission ratio, \mathcal{T} , which was stable to better than 10^{-6} . The incident power is actively controlled using the level on PD A while the frequency of the incident light is set with an absolute uncertainty of 2 kHz, limited by our ability to realize the unperturbed transition frequency of the Cs saturated absorption feature to which the master laser was locked. Precision in the radio frequency (RF) frequency detuning between the master and probe lasers was ensured by referencing the offset-frequency locking electronics to a Cs beam clock-disciplined maser. Technical details about the apparatus are given in the Supplementary Methods section.

References

- Fellmuth, B., Gaiser, C. & Fischer, J. Determination of the Boltzmann constant—status and prospects. *Meas. Sci. Technol.* **17**, R145–R159 (2006).
- Stewart, G., Johnstone, W., Bain, J. R. P., Ruxton, K. & Duffin, K. Recovery of absolute gas absorption line shapes using tunable diode laser spectroscopy with wavelength modulation—part I: Theoretical analysis. *J. Lightwave Technol.* **29**, 811–821 (2011).
- Drossart, P. Infrared spectroscopy of planetary atmospheres. *C. R. Phys.* **6**, 817–824 (2005).
- Koch, J. A. *et al.* High-resolution spectroscopy for doppler-broadening ion temperature measurements of implosions at the national ignition facility. *Rev. Sci. Instrum.* **83**, 10E127-1–10E127-3 (2012).
- Grefenstette, B. W. *et al.* Asymmetries in core-collapse supernovae from maps of radioactive ^{44}Ti in Cassiopeia A. *Nature* **506**, 339–342 (2014).

6. Hayato, A. *et al.* Expansion velocity of ejecta in Tycho's supernova remnant measured by doppler broadened x-ray line emission. *Astrophys. J.* **725**, 894 (2010).
7. Wood, C. S. *et al.* Measurement of parity nonconservation and an anapole moment in cesium. *Science* **275**, 1759–1763 (1997).
8. Jönsson, P. *et al.* Large-scale multiconfiguration Hartree-Fock and configuration-interaction calculations of the transition probability and hyperfine structures in the sodium resonance transition. *Phys. Rev. A* **53**, 4021–4030 (1996).
9. Brage, T., Fischer, C. F. & Jönsson, P. Effects of core-valence and core-core correlation on the line strength of the resonance lines in Li I and Na I. *Phys. Rev. A* **49**, 2181–2184 (1994).
10. Bordé, C. J. Base units of the SI, fundamental constants and modern quantum physics. *Phil. Trans. R. Soc. A* **363**, 2177–2201 (2005).
11. Bordé, C. J. Theory of linear absorption line shapes in gases. *C. R. Phys.* **10**, 866 (2009).
12. Moldover, M. R., Trusler, J. P. M., Edwards, T. J., Mehl, J. B. & Davis, R. S. Measurement of the universal gas constant r using a spherical acoustic resonator. *Phys. Rev. Lett.* **60**, 249–252 (1988).
13. Pitre, L. *et al.* Measurement of the Boltzmann constant k_B using a quasi-spherical acoustic resonator. *Int. J. Thermophys.* **32**, 1825–1886 (2011).
14. de Podesta, M. *et al.* A low-uncertainty measurement of the Boltzmann constant. *Metrologia* **50**, 354 (2013).
15. Cohen, E. R. & DuMond, J. W. M. Our knowledge of the fundamental constants of physics and chemistry in 1965. *Rev. Mod. Phys.* **37**, 537–594 (1965).
16. Daussy, C. *et al.* Direct determination of the Boltzmann constant by an optical method. *Phys. Rev. Lett.* **98**, 250801 (2007).
17. Casa, G. *et al.* Primary gas thermometry by means of laser-absorption spectroscopy: determination of the Boltzmann constant. *Phys. Rev. Lett.* **100**, 200801 (2008).
18. Triki, M. *et al.* Speed-dependent effects in NH_3 self-broadened spectra: Towards the determination of the Boltzmann constant. *Phys. Rev. A* **85**, 062510 (2012).
19. Lemarchand, C. *et al.* High precision line shape studies in low pressure ammonia for an accurate determination of the Boltzmann constant. *J. Phys. Conf. Ser.* **397**, 012028 (2012).
20. Cygan, A., Lisak, D., Trawiński, R. S. & Ciurylo, R. Influence of the line-shape model on the spectroscopic determination of the Boltzmann constant. *Phys. Rev. A* **82**, 032515 (2010).
21. Hald, J., Nielsen, L., Petersen, J. C., Varming, P. & Pedersen, J. E. Fiber laser optical frequency standard at 1.54 μm . *Opt. Express* **19**, 2052–2063 (2011).
22. Gianfrani, L. Highly-accurate line shape studies in the near-IR spectrum of H_2^{18}O . Implications for the spectroscopic determination of the Boltzmann constant. *J. Phys. Conf. Ser.* **397**, 012029 (2012).
23. Truong, G.-W., Anstie, J. D., May, E. F., Stace, T. M. & Luiten, A. N. Absolute absorption line-shape measurements at the shot-noise limit. *Phys. Rev. A* **86**, 030501 (2012).
24. Truong, G.-W., May, E. F., Stace, T. M. & Luiten, A. N. Quantitative atomic spectroscopy for primary thermometry. *Phys. Rev. A* **83**, 033805 (2011).
25. Stace, T. M., Truong, G.-W., Anstie, J., May, E. F. & Luiten, A. N. Power-dependent line-shape corrections for quantitative spectroscopy. *Phys. Rev. A* **86**, 012506 (2012).
26. Stace, T. M. & Luiten, A. N. Theory of spectroscopy in an optically pumped effusive vapor. *Phys. Rev. A* **81**, 033848 (2010).
27. Truong, G.-W. *et al.* Atomic spectroscopy for primary thermometry. *Metrologia*. **52**, S324 (2015).
28. Moretti, L. *et al.* Determination of the Boltzmann constant by means of precision measurements of H_2^{18}O line shapes at 1.39 μm . *Phys. Rev. Lett.* **111**, 060803 (2013).
29. Lemarchand, C. *et al.* Determination of the Boltzmann constant by laser spectroscopy as a basis for future measurements of the thermodynamic temperature. *Int. J. Thermophys.* **31**, 1347–1359 (2010).
30. Djerroud, K. *et al.* Measurement of the Boltzmann constant by the Doppler broadening technique at a 3.8×10^{-5} accuracy level. *C. R. Phys.* **10**, 883 (2009).
31. Gerginov, V. *et al.* Optical frequency measurements of $6s\ ^2s_{1/2}-6p\ ^2P_{1/2}(d_1)$ transitions in ^{133}Cs and their impact on the fine-structure constant. *Phys. Rev. A* **73**, 032504 (2006).
32. Rafac, R. J., Tanner, C. E., Livingston, A. E. & Berry, H. G. Fast-beam laser lifetime measurements of the cesium $6p\ ^2P_{1/2,3/2}$ states. *Phys. Rev. A* **60**, 3648–3662 (1999).
33. Amini, J. M. & Gould, H. High precision measurement of the static dipole polarizability of cesium. *Phys. Rev. Lett.* **91**, 153001 (2003).
34. Vadla, C., Horvatic, V. & Niemax, K. Accurate determination of the atomic number density in dense Cs vapors by absorption measurements of Cs_2 triplet bands. *Appl. Phys. B* **84**, 523–527 (2006).
35. Steck, D. A. Cesium D Line Data. Available at <http://steck.us/alkalidata> (revision 2.1.4) accessed on 23 December 2010.
36. Biercuk, M. *et al.* Optimized dynamical decoupling in a model quantum memory. *Nature* **458**, 996–1000 (2009).
37. Roger, C. *et al.* Quantum interference and light polarization effects in unresolvable atomic lines: Application to a precise measurement of the $^6\text{Li}\ D_2$ lines. *Phys. Rev. A* **87**, 032504 (2013).
38. Horbatsch, M. & Hessels, E. A. Shifts from a distant neighboring resonance. *Phys. Rev. A* **82**, 052519 (2010).
39. Horbatsch, M. & Hessels, E. A. Shifts from a distant neighboring resonance for a four-level atom. *Phys. Rev. A* **84**, 032508 (2011).
40. Marsman, A., Horbatsch, M. & Hessels, E. A. Shifts due to distant neighboring resonances for laser measurements of 2^3S_1 -to- 2^3P_j transitions of helium. *Phys. Rev. A* **86**, 040501 (2012).
41. Stace, T. M. Quantum limits of thermometry. *Phys. Rev. A* **82**, 011611 (2010).

Acknowledgements

The authors wish to thank the NIST Precision Measurement Grants Program, the Australian Research Council through the CE110001013, FT0991631 and DP1094500 grants for funding this work. The authors also wish to acknowledge the South Australian Government who have provided generous financial support through the Premier's Science and Research Fund. We thank Michael Moldover and Greg Strouse of NIST, and Mark Ballico from NMI Australia, for their contributions to the SPRT thermometry.

Author contributions

G.-W.T. co-constructed the experimental apparatus and co-analysed the data under the supervision of A.N.L., E.F.M., J.D.A. and T.M.S. T.M.S. and A.N.L. developed the Voigt lineshape correction framework and co-analysed the data. J.D.A. co-constructed the thermal isolation apparatus. E.F.M. provided expertise in SPRT usage and precision resistance thermometry. All authors contributed equally to the manuscript and the Supplementary Information.

Additional information

Supplementary Information accompanies this paper at <http://www.nature.com/naturecommunications>

Competing financial interests: The authors declare no competing financial interests.

Reprints and permission information is available online at <http://npg.nature.com/reprintsandpermissions/>

How to cite this article: Truong, G.-W. *et al.* Accurate lineshape spectroscopy and the Boltzmann constant. *Nat. Commun.* 6:8345 doi: 10.1038/ncomms9345 (2015).



This work is licensed under a Creative Commons Attribution 4.0 International License. The images or other third party material in this article are included in the article's Creative Commons license, unless indicated otherwise in the credit line; if the material is not included under the Creative Commons license, users will need to obtain permission from the license holder to reproduce the material. To view a copy of this license, visit <http://creativecommons.org/licenses/by/4.0/>